

Change of Nano Material Electrical Characteristics for Medical System Applications [Corrigendum]

Chen P, Zhang X, Jiang K, et al. *Int J Nanomedicine*. 2019;14:10119–10122.

Page 10120, left column, Materials And Methods section, line 2, the text “30 ~ 50 nm thick” should read “30 ~ 60 nm thick”.

Page 10120, Figure 2, the Y axis “ $I_{DS}(nA)$ ” should read “ $I_{DS}(pA)$ ”.

Figure 3 on page 10120, the authors have advised the figure was created using the wrong sample and therefore, is incorrect. The correct Figure 3 is shown below.

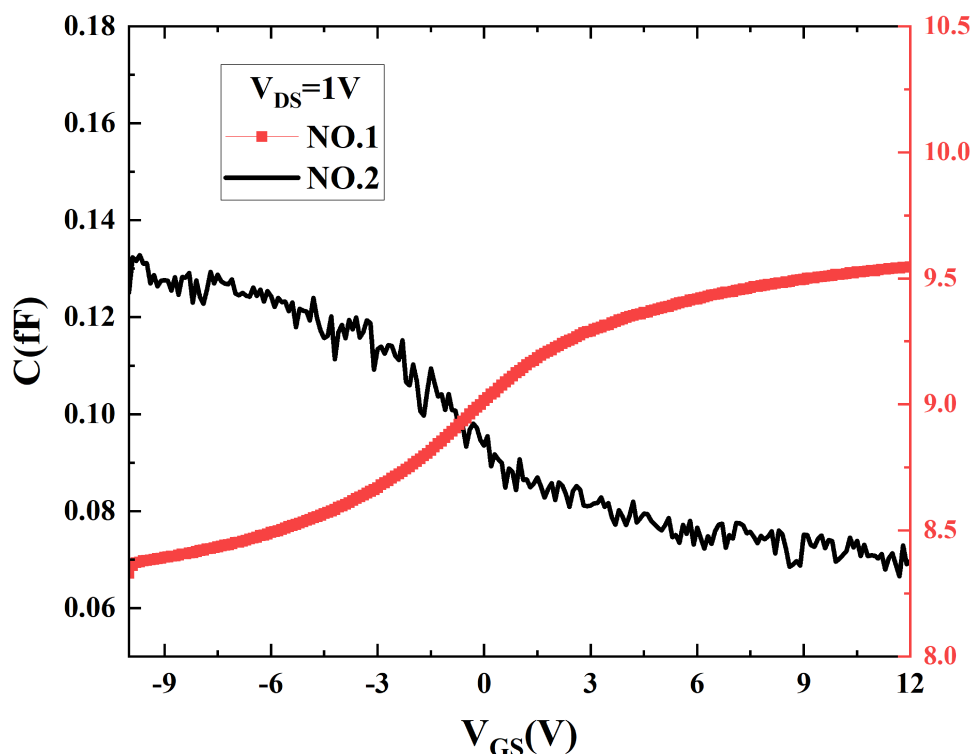


Figure 3 The C-V curve of the present n-type TFTs could be easily changed to that of p-type TFTs.

The authors apologize for these errors and advise they do not affect the results of the paper.

International Journal of Nanomedicine**Dovepress****Publish your work in this journal**

The International Journal of Nanomedicine is an international, peer-reviewed journal focusing on the application of nanotechnology in diagnostics, therapeutics, and drug delivery systems throughout the biomedical field. This journal is indexed on PubMed Central, MedLine, CAS, SciSearch®, Current Contents®/Clinical Medicine, Journal Citation Reports/Science Edition, EMBase, Scopus and the Elsevier Bibliographic databases. The manuscript management system is completely online and includes a very quick and fair peer-review system, which is all easy to use. Visit <http://www.dovepress.com/testimonials.php> to read real quotes from published authors.

Submit your manuscript here: <https://www.dovepress.com/international-journal-of-nanomedicine-journal>

<https://doi.org/10.2147/IJN.S386292>