



# Differences in the Measurement of Functional Residual Capacity Between Body Plethysmographs of Two Manufacturers

Peter Alter <sup>1</sup>, Jan Orszag<sup>2,3</sup>, Emiel FM Wouters<sup>4,5</sup>, Claus F Vogelmeier<sup>1</sup>, Rudolf A Jörres <sup>2</sup>

<sup>1</sup>Department of Medicine, Pulmonary and Critical Care Medicine, Philipps-University of Marburg (UMR), Germany, Member of the German Center for Lung Research (DZL), Marburg, Germany; <sup>2</sup>Institute and Outpatient Clinic for Occupational, Social and Environmental Medicine, University Hospital, LMU Munich, Comprehensive Pneumology Center Munich (CPC-M), Member of the German Center for Lung Research (DZL), Munich, Germany; <sup>3</sup>Department of Anaesthesiology, University Hospital, LMU Munich, Munich, Germany; <sup>4</sup>Department of Respiratory Medicine, Maastricht University Medical Centre, Maastricht, Netherlands; <sup>5</sup>Ludwig Boltzmann Institute for Lung Health, Vienna, Austria

Correspondence: Peter Alter, Department of Medicine, Pulmonary and Critical Care Medicine, Philipps-University of Marburg (UMR), Baldingerstrasse, Marburg, 35033, Germany, Email [Alter@uni-marburg.de](mailto:Alter@uni-marburg.de)

**Abstract:** Body plethysmography is a fundamental method for the assessment of static lung volumes. Although equipment is provided by several manufacturers, there are no established cross-vendor tools for quality control. In the process of quality control and analysis of data on hyperinflation from the large COPD cohort COSYCONET, hints appeared that plethysmographs of different vendors might yield different values for static lung volumes. Functional residual capacity (FRC) differed about 0.67 litres between plethysmographs of the manufacturer Vyair and Ganshorn. Absolute differences of residual lung volume (RV) and total lung capacity (TLC) were similar. It appears undeniable that differences of this magnitude have an impact on clinical interpretation. Thus, device harmonization seems to be required.

**Keywords:** lung function, body plethysmography, static lung volumes, functional residual capacity

## Introduction

Body plethysmography is a major tool in the inventory of lung function measurements and suited for the assessment of static lung volumes, especially functional residual capacity (FRC), residual volume (RV) and total lung capacity (TLC). Its physiological basis and practical implementation have been described in detail.<sup>1</sup> Equipment is provided by a number of manufacturers. There seem to be no independent devices for quality control to be used by all manufacturers. In view of the intricacies of the method, one has to consider the possibility that plethysmographs of different manufacturers show systematic differences in measured values.

In the multicenter COPD cohort COSYCONET (COPD and Systemic Consequences - Comorbidities Network), body plethysmography is part of assessments.<sup>2</sup> In the process of quality control and analysis, more and more hints appeared that plethysmographs of different manufacturers located at different participating study centers might yield different values for FRC and derived parameters.<sup>3,4</sup> This raised the question, whether suspected differences between devices could be verified, whether it reached relevant magnitude, and which factors might be responsible. If such differences should exist and exceed a certain magnitude, they might have consequences with regard to the applicability of reference values, irrespective of the use of ECSC (European community for coal and steel)<sup>5</sup> or more recent equations.<sup>6,7</sup>

## Methods

Data from COSYCONET were used. Anthropometric, clinical and functional data including spirometry (forced expiratory volume in 1 s, FEV<sub>1</sub>; forced vital capacity, FVC) and body plethysmography (FRC, RV, TLC) were obtained following standardized protocols in 30 study centres throughout Germany.<sup>2</sup> The study protocol was approved by the

Ethical Committees of all centres, and all participants gave their written informed consent. The study was performed in accordance with the declaration of Helsinki. ClinicalTrials.gov: NCT01245933.

The centres using a plethysmograph of the manufacturer Vyair (CareFusion, Jaeger; Höchberg, Germany) provided data from 1988 COPD patients of GOLD grades 1–4<sup>8</sup> as described previously (38.1% female, mean (SD) age 65.1±8.4 years, GOLD grades 1/2/3/4: 9.4/42.6/38.5/9.5%).<sup>4</sup> Additionally, we included 156 patients (51.9% female, mean (SD) age 64.1±9.2 years, GOLD grades: 1/2/3/4: 8.3/46.8/33.3/11.5%) from one centre using a Ganshorn (Niederlauer, Germany) plethysmograph, applying the same criteria of data validity and completeness.<sup>4</sup> Thus, the present analysis included 2144 patients.

Analysis of baseline characteristics and comparison among both groups was performed (Table 1). As we did not measure the same patient in both plethysmographs, we then performed linear regression analyses of static lung volumes (FRC, RV, TLC), either as % predicted<sup>9</sup> or as absolute values in litres, as well as of RV/TLC %. As previously,<sup>4</sup> predictors were FEV<sub>1</sub> and FVC, both as % predicted,<sup>10</sup> sex, age, height and body mass index (BMI), and introducing an indicator variable for the type of plethysmograph. The magnitude of the respective regression coefficient would then indicate the difference between devices after adjustment for anthropometric and spirometric characteristics.

## Results


Analysis of the group of 156 patients showed that the relationship between predictors, especially FEV<sub>1</sub> and FVC, and RV/TLC % was the same as in the larger group,<sup>4</sup> thus patients did not appear to be qualitatively different and the pooled analysis was valid. Regarding RV/TLC %, it revealed a significantly ( $p < 0.001$  each) smaller average value in the 156 patients ( $\Delta = -6.9$ ; 95% CI:  $-7.9$ ;  $-5.8$ ). The same was true for % predicted values of FRC ( $\Delta = -20.9$ ; 95% CI:  $-25.4$ ;  $-16.4$ ), RV ( $\Delta = -34.0$ ; 95% CI:  $-40.5$ ;  $-27.6$ ), and TLC ( $\Delta = -10.2$ ; 95% CI:  $-12.7$ ;  $-7.7$ ), and for the absolute values in litres of FRC ( $\Delta = -0.67$ ; 95% CI:  $-0.82$ ;  $-0.53$ ; Figure 1), RV ( $\Delta = -0.77$ ; 95% CI:  $-0.92$ ;  $-0.63$ ), and TLC ( $\Delta = -0.61$ ; 95% CI:  $-0.77$ ;  $-0.46$ ). Details are shown in Table 2.

## Discussion

In the present analysis we addressed the question, whether body plethysmographs of two manufacturers showed systematic differences in the measured values of static lung volumes. Indeed, there were such differences. In direct comparison, the Ganshorn device yielded lower and the Vyair devices higher values of static lung volumes, especially functional residual capacity (FRC). These findings were obtained via regression analysis, adjusting for patient characteristics known to affect lung volumes.<sup>3</sup> Notably, they were consistent regarding both absolute values and values in % predicted. The absolute differences of FRC, RV and TLC between plethysmographs were similar, with large overlap of confidence intervals, indicating that the 0.67 L difference in FRC translated into parallel differences in RV and TLC. As usual, these parameters were derived from FRC via consecutive breathing maneuvers involving the expiratory reserve volume (ERV) and the inspiratory vital capacity (VCin). It is clear that % predicted values differed as they depended on the volumes used for reference; they reached average values of about 21% for FRC, 34% for RV and 10% for TLC. It seems difficult to deny that differences of this magnitude are relevant, both as absolute values and as % predicted. Apart from the variability arising from the choice of reference equations, such differences are likely to affect the interpretation of plethysmographic results, potentially leading to marked over- or underestimation of hyperinflation depending on the device used.

**Table 1** Baseline Characteristics

	Jaeger n = 1988	Ganshorn n = 156	p value
<b>GOLD grades 1/2/3/4</b>	187/847/766/188 (9.4/42.6/38.5/9.5%)	13/73/52/18 (8.3/46.8/33.3/11.5%)	0.485
<b>Age [years]</b>	65.1 ± 8.4	64.1 ± 9.2	0.184
<b>Height [cm]</b>	171 ± 9	171 ± 10	0.840
<b>BMI [kg/m<sup>2</sup>]</b>	26.6 ± 5.2	26.5 ± 4.9	0.791
<b>Sex [male/female]</b>	1231 (61.9%)/757 (38.1%)	75 (48.1%)/81 (51.9%)	<0.001

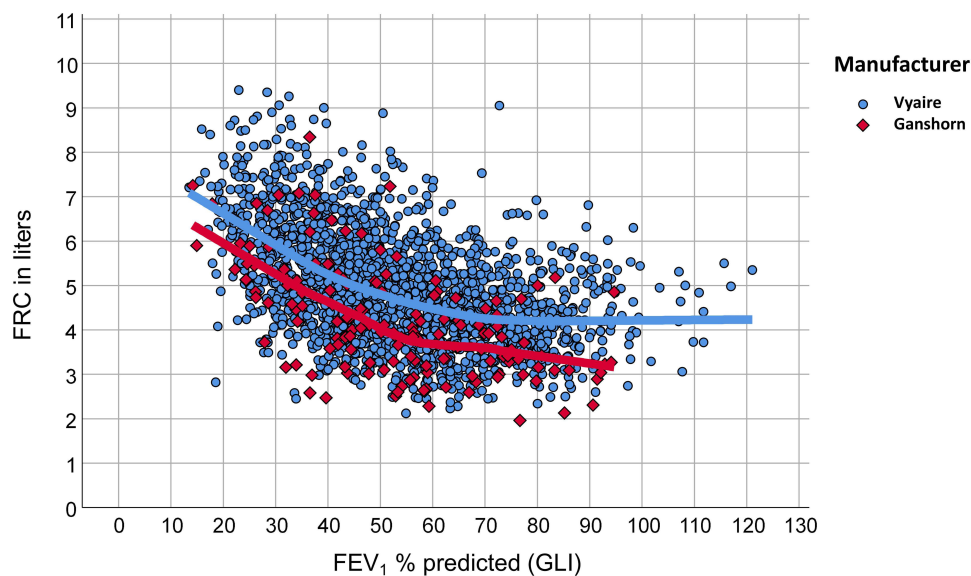

**Figure 1** Difference in FRC between body plethysmographs. The horizontal axis shows FEV<sub>1</sub> % predicted (GLI), the vertical axis FRC in litres measured by either the Vyair (blue circles, n=1988) or the Ganshorn (red diamonds, n=156) plethysmograph. Additionally, LOESS fit lines are shown for both groups in the respective colors, indicating a difference of more than 0.5 litres between FRC values at a given value of FEV<sub>1</sub> % predicted. When residual terms after adjustment for FEV<sub>1</sub>, FVC, sex, age, height and BMI were used, essentially the same picture was obtained, with the difference that the dependence on FEV<sub>1</sub> disappeared. This demonstrated that the difference shown in the graph was not due to residual confounding but a robust result even in unadjusted data.

It is unlikely that the observed differences are confined to the equipment of just the two manufacturers chosen. Their occurrence and magnitude could depend on factors involving hardware, software and the manner the shutter manoeuvre is performed. There are no obligatory calibration devices to be used by all manufacturers. We consider differences in software to be more likely and better amenable to future standardization. The shutter manoeuvre is usually performed at the end of normal tidal expiration, or shortly thereafter, with correction for the inspired volume. To our knowledge, in most plethysmographs, FRC is taken as that volume, while in others half of the tidal volume is added. While this might be adequate regarding the computation of airway resistance (Raw) from specific airway resistance (sRaw) as a value averaged over the breathing cycle, it implies a difference in FRC, and consequently in the computed Raw.<sup>1</sup> According to our experience, actual tidal volume may be as large as 1.0 or 1.5 L, despite the fact that more shallow breathing is recommended, thus a numerical difference of 0.67 L may easily be introduced. We also were informed by manufacturers on differences in the advice given to patients prior to the shutter manoeuvre which could affect FRC by promoting changes in lung volumes. In the present analysis, we cannot resolve these issues but the fact of large differences in FRC and derived volumes is not affected. It also has to be noted that the measurements in all study centers were performed did not involve any unusual procedures and were performed in accordance with both guidelines and what we know from clinical routine procedures. Thus, they have impact for clinical practice not just the cohort study from which the data used in this analysis were taken.

Our findings reveal a source of variation in body plethysmographic results that should ameliorated by harmonization between manufacturers. Variations of the observed magnitude hamper the usefulness of body plethysmography, and we believe that clinicians and researchers should be aware of this in order to exploit the full potential of this powerful lung function tool.

## Take Home Message

Body plethysmographs of two manufacturers showed marked differences in the measured values of static lung volumes that likely to have an impact on clinical interpretation. Some harmonization seems needed.

## COSYCONET Study Group

Andreas, Stefan (Lungenfachklinik, Immenhausen); Bals, Robert Universitätsklinikum des Saarlandes); Behr, Jürgen and Kahnert, Kathrin (Klinikum der Ludwig-Maximilians-Universität München); Bahmer, Thomas (Universitätsklinikum

**Table 2** Results from Multivariate Regression Analyses of the Dependent Variables Given in the Top Row and the Predictors Given Below

Predictors	RV/TLC [%]	FRC %Predicted	RV %Predicted	TLC %Predicted	FRC [l]	RV [l]	TLC [l]
<b>FEV<sub>1</sub> %pred</b>	-0.2 [-0.2; -0.2]	-1.4 [-1.5; -1.3]	-1.5 [-1.7; -1.4]	-0.6 [-0.6; -0.5]	-0.05 [-0.05; -0.04]	-0.04 [-0.04; -0.03]	-0.04 [-0.04; -0.03]
<b>FVC %pred</b>	-0.2 [-0.3; -0.2]	0.5 [0.4; 0.6]	-0.1 [-0.2; 0.1]	0.5 [0.5; 0.6]	0.02 [0.02; 0.02]	0.00 [0.00; 0.00]	0.03 [0.03; 0.04]
<b>Age [years]</b>	0.3 [0.2; 0.3]	-0.1 [-0.3; 0.0]	-1.0 [-1.2; -0.8]	-0.2 [-0.3; -0.2]	0.00 [0.00; 0.01]	0.01 [0.01; 0.02]	-0.02 [-0.02; -0.01]
<b>Height [cm]</b>	-0.1 [-0.2; -0.1]	0.3 [0.1; 0.5]	0.2 [-0.1; 0.4]	-0.2 [-0.3; -0.1]	0.04 [0.04; 0.05]	0.03 [0.02; 0.04]	0.07 [0.07; 0.08]
<b>BMI [kg/m<sup>2</sup>]</b>	-0.2 [-0.2; -0.1]	-1.4 [-1.7; -1.2]	-1.3 [-1.6; -1]	-0.4 [-0.6; -0.3]	-0.05 [-0.05; -0.04]	-0.03 [-0.04; -0.02]	-0.03 [-0.03; -0.02]
<b>Sex [female vs male]</b>	3.1 [2.3; 3.8]	15.2 [11.9; 18.5]	14.2 [9.4; 18.9]	7.8 [5.9; 9.7]	-0.43 [-0.53; -0.32]	-0.24 [-0.35; -0.13]	-0.81 [-0.93; -0.70]
<b>Plethysmograph [Ganshorn vs Jaeger]</b>	-6.9 [-7.9; -5.8]	-20.9 [-25.4; -16.4]	-34.0 [-40.5; -27.6]	-10.2 [-12.7; -7.7]	-0.67 [-0.82; -0.53]	-0.77 [-0.92; -0.63]	-0.61 [-0.77; -0.46]

**Notes:** Non-standardized regression coefficients and their 95% confidence intervals are given. % predicted refers to GLI reference values. Please note that the differences between plethysmographs regarding the absolute volumes are of similar magnitude and that their confidence intervals overlap, indicating that the difference regarding FRC is that which determined those regarding RV and TLC as derived parameters.

**Abbreviations:** FRC, functional residual capacity; RV, residual volume; TLC, total lung capacity.

Schleswig Holstein) and Bewig, Burkhard (Städtisches Krankenhaus Kiel); Ewert, Ralf and Stubbe, Beate (Universitätsmedizin Greifswald); Ficker, Joachim H. (Klinikum Nürnberg, Paracelsus Medizinische Privatuniversität Nürnberg); Grohé, Christian (Ev. Lungenklinik Berlin); Held, Matthias (Klinikum Würzburg Mitte gGmbH, Standort Missioklinik); Behr, Jürgen and Henke, Markus (Asklepios Fachkliniken München-Gauting); Herth, Felix (Thoraxklinik Heidelberg gGmbH); Kirsten, Anne-Marie and Watz, Henrik (Pneumologisches Forschungsinstitut an der Lungenclinic Grosshansdorf GmbH); Koczulla, Rembert (Schön Klinik Berchtesgadener Land); Kronsbein, Juliane (Berufsgenossenschaftliches Universitätsklinikum Bergmannsheil, Bochum); Kropf-Sanchen, Cornelia (Universitätsklinikum Ulm); Herzmann, Christian (Forschungszentrum Borstel); Pfeifer, Michael (Klinik Donaustauf); Randerath, Winfried J. (Wissenschaftliches Institut Bethanien e. V., Solingen); Seeger, Werner (Justus-Liebig-Universität Gießen); Studnicka, Michael (Uniklinikum Salzburg); Taube, Christian (Ruhrländklinik gGmbH Essen); Timmermann, Hartmut (Hamburger Institut für Therapieforchung GmbH); Alter, Peter; Schmeck, Bernd and Vogelmeier, Claus (Universitätsklinikum Gießen und Marburg GmbH, Standort Marburg); Welte, Tobias (Medizinische Hochschule Hannover); Wirtz, Hubert (Universitätsklinikum Leipzig).

The study was based on 2741 patients recruited within the COSYCONET framework (ClinicalTrials.gov, Identifier: NCT01245933). For further information see Karch A, Vogelmeier C, Welte T, Bals R, Kauczor HU, Biederer J, Heinrich J, Schulz H, Glaser S, Holle R et al.: The German COPD cohort COSYCONET: Aims, methods and descriptive analysis of the study population at baseline. *Respir Med* 2016, 114:27–37.

## Data Sharing Statement

The basic data are part of the German COPD cohort COSYCONET ([www.asconet.net](http://www.asconet.net)) and available upon request. The website of the network provides a detailed procedure for respective applications. The data can be obtained after submission of a proposal that is evaluated by the steering committee. Qualified requests should be addressed to: Mrs Inge Kokot, Competence Network Asthma and COPD, Philipps-University of Marburg, Email: kokot@asconet.net

All results to which the manuscript refers are documented appropriately in the text, figures or tables.

## Ethics Approval and Consent to Participate

COSYCONET was approved by the ethical committees of all study centres and all patients gave written informed consent. The study was performed in accordance with the declaration of Helsinki.

## Acknowledgments

We are grateful to all COSYCONET study centres, especially to all study nurses, for their excellent and enduring work in data collection, as well as to all patients who were willing to participate in this study.

## Author Contributions

All authors made a significant contribution to the work reported, whether that is in the conception, study design, execution, acquisition of data, analysis and interpretation, or in all these areas; took part in drafting, revising or critically reviewing the article; gave final approval of the version to be published; have agreed on the journal to which the article has been submitted; and agree to be accountable for all aspects of the work.

## Funding

COSYCONET is supported by the German Federal Ministry of Education and Research (BMBF) Competence Network Asthma and COPD (ASCONET) and performed in collaboration with the German Center for Lung Research (DZL). The project is funded by the BMBF with grant number 01 GI 0881, and is supported by unrestricted grants from AstraZeneca GmbH, Bayer Schering Pharma AG, Boehringer Ingelheim Pharma GmbH & Co. KG, Chiesi GmbH, GlaxoSmithKline, Grifols Deutschland GmbH, MSD Sharp & Dohme GmbH, Mundipharma GmbH, Novartis Deutschland GmbH, Pfizer Pharma GmbH, Takeda Pharma Vertrieb GmbH & Co. KG, Teva GmbH for patient investigations and laboratory

measurements. J.V. is supported by the NIHR Manchester Biomedical Research Centre. The funding body had no involvement in the design of the study, or the collection, analysis or interpretation of the data.

## Disclosure

Peter Alter declares no relevant competing interests. Jan Orszag declares no relevant competing interests. Emiel F. M. Wouters declares no relevant competing interests. Claus F. Vogelmeier declares grants or contracts to his institution from the German Ministry of Education and Science (BMBF), AstraZeneca, Boehringer Ingelheim, GlaxoSmithKline, Grifols, and Novartis, consulting fees from AstraZeneca, Boehringer Ingelheim, CSL Behring, Chiesi, GlaxoSmithKline, Menarini, Novartis, and Nuaira, MedUpdate, payment or honoraria for lectures, presentations, speakers bureaus, manuscript writing or educational events from Aerogen, AstraZeneca, Boehringer Ingelheim, CSL Behring, Chiesi, GlaxoSmithKline, Menarini, and Novartis, all of which are outside the scope of the submitted work. Rudolf A. Jörres declares no relevant competing interests.

## References

1. Criece CP, Sorichter S, Smith HJ, et al. Body plethysmography—its principles and clinical use. *Respir Med.* 2011;105(7):959–971. doi:10.1016/j.rmed.2011.02.006
2. Karch A, Vogelmeier C, Welte T, et al. The German COPD cohort COSYCONET: aims, methods and descriptive analysis of the study population at baseline. *Respir Med.* 2016;114:27–37. doi:10.1016/j.rmed.2016.03.008
3. Alter P, Rabe KF, Schulz H, Vogelmeier CF, Jorres RA. Influence of body mass on predicted values of static hyperinflation in COPD. *Int J Chron Obstruct Pulmon Dis.* 2018;13:2551–2555. doi:10.2147/COPD.S164096
4. Alter P, Orszag J, Kellerer C, et al. Prediction of air trapping or pulmonary hyperinflation by forced spirometry in COPD patients: results from COSYCONET. *ERJ Open Res.* 2020;6(3):00092–2020. doi:10.1183/23120541.00092-2020
5. Quanjer PH. Standardized lung function testing: report working party Standardization of lung function tests. Published in 1983 in Luxembourg by European community for coal and steel; 1983.
6. Garcia-Rio F, Dorgham A, Pino JM, Villasante C, Garcia-Quero C, Alvarez-Sala R. Lung volume reference values for women and men 65 to 85 years of age. *Am J Respir Crit Care Med.* 2009;180(11):1083–1091. doi:10.1164/rccm.200901-0127OC
7. Koch B, Friedrich N, Volzke H, et al. Static lung volumes and airway resistance reference values in healthy adults. *Respirology.* 2013;18(1):170–178. doi:10.1111/j.1440-1843.2012.02268.x
8. Vogelmeier CF, Criner GJ, Martinez FJ, et al. Global strategy for the diagnosis, management, and prevention of chronic obstructive lung disease 2017 report: GOLD executive summary. *Eur Respir J.* 2017;49(3):1700214. doi:10.1183/13993003.00214-2017
9. Quanjer PH, Tammeling GJ, Cotes JE, Pedersen OF, Peslin R, Yernault JC. Lung volumes and forced ventilatory flows. Report working party standardization of lung function tests, European community for steel and coal. Official statement of the European Respiratory Society. *Eur Respir J Suppl.* 1993;6(Suppl 16):5–40. doi:10.1183/09041950.005s1693
10. Quanjer PH, Stanojevic S, Cole TJ, et al. Multi-ethnic reference values for spirometry for the 3–95-yr age range: the global lung function 2012 equations. *Eur Respir J.* 2012;40(6):1324–1343. doi:10.1183/09031936.00080312

International Journal of Chronic Obstructive Pulmonary Disease

Dovepress

Publish your work in this journal

The International Journal of COPD is an international, peer-reviewed journal of therapeutics and pharmacology focusing on concise rapid reporting of clinical studies and reviews in COPD. Special focus is given to the pathophysiological processes underlying the disease, intervention programs, patient focused education, and self management protocols. This journal is indexed on PubMed Central, MedLine and CAS. The manuscript management system is completely online and includes a very quick and fair peer-review system, which is all easy to use. Visit <http://www.dovepress.com/testimonials.php> to read real quotes from published authors.

Submit your manuscript here: <https://www.dovepress.com/international-journal-of-chronic-obstructive-pulmonary-disease-journal>